


## ISO 3664:2009 Messprotokoll

Prüfbericht gemäß ISO 3664:2009

Datum : 2017-09-01 12:18:06  
 Abstimmplatz : 2XPC, moduLight-Leuchte  
 Firma : JUST Normlicht GmbH

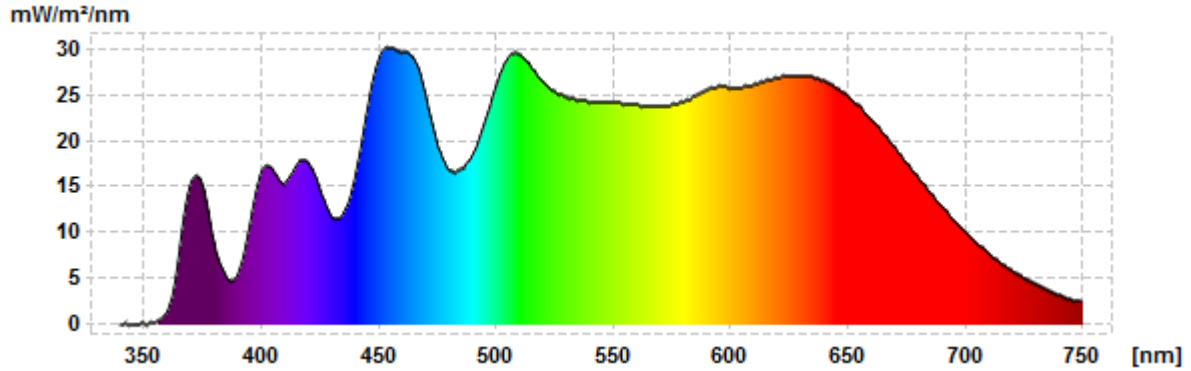

<p>11</p> <p>Y = 89% =&gt; PASS</p>	<p>12</p> <p>Y = 95% =&gt; PASS</p>	<p>13</p> <p>Y = 88% =&gt; PASS</p>
<p>21</p> <p>Y = 95% =&gt; PASS</p>	<p>22</p> <p>Y = 1992,55 lx =&gt; PASS                  Ch Err = 0,004 =&gt; PASS                  Ra = 96,6 =&gt; PASS                  Ri &gt;= 93,9 =&gt; PASS                  Mlvis = 0,4 =&gt; PASS                  Mluv = 0,7 =&gt; PASS</p>	<p>23</p> <p>Y = 95% =&gt; PASS</p>
<p>31</p> <p>Y = 88% =&gt; PASS</p>	<p>32</p> <p>Y = 92% =&gt; PASS</p>	<p>33</p> <p>Y = 87% =&gt; PASS</p>

**Metamerism Indices**

Mlvis = 0,40  
 Mluv = 0,70

**Metamerism Indices**

Ra = 96,6 => PASS  
 R1 = 95,2 => PASS  
 R2 = 97,5 => PASS  
 R3 = 99,0 => PASS  
 R4 = 93,9 => PASS  
 R5 = 95,1 => PASS  
 R6 = 95,1 => PASS  
 R7 = 99,5 => PASS  
 R8 = 97,7 => PASS

**Certification according to ISO 3664:2009 PASS**